


Quantaurus-QY[®]

Absolute PL quantum yield spectrometer C11347 series

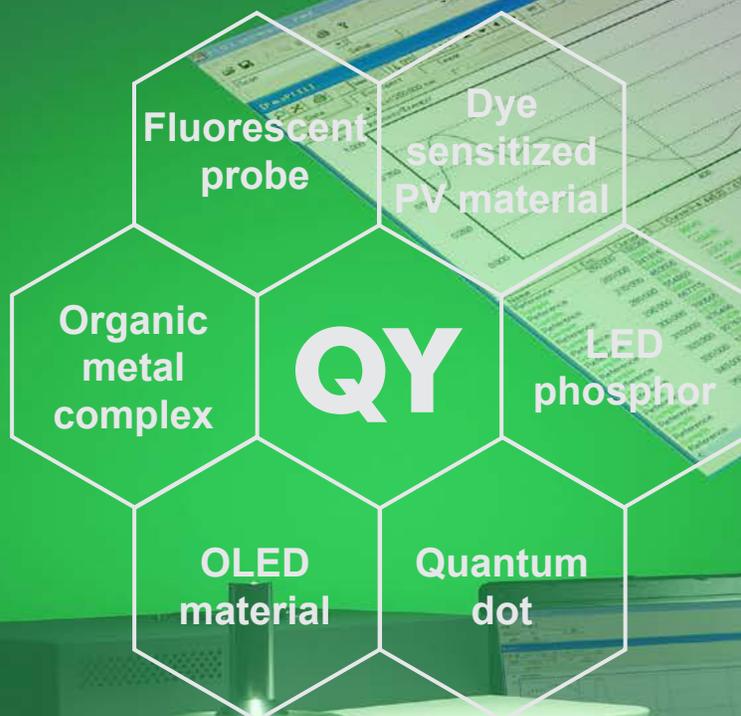

HAMAMATSU

PHOTON IS OUR BUSINESS

Quantaurs-QY was developed as a compact, easy-to-use system with a small footprint based on Hamamatsu's established C9920-02,-02G/03,-03G systems for measuring absolute photoluminescence quantum yields. Operating this system is simple. Load a sample and press the start button to measure the photoluminescence quantum yields, excitation wavelength dependence, PL excitation spectrum and other properties in a short time.



QY Absolute PL Quantum Yield

Measuring absolute photoluminescence quantum yields (internal quantum efficiency) of light-emitting materials

In developing new light-emitting materials, it is essential to improve their photoluminescence efficiency.

Improving this efficiency requires accurate techniques for measuring the quantum yield. Quantaurs-QY includes an excitation light source consisting of a xenon lamp and a monochromator, an integration sphere with optional nitrogen gas flow, and a multichannel detector capable of simultaneous multi-wavelength measurement, which are all integrated into a single package. The system utilizes dedicated software for making the measurements. The detector is a cooled, back-thinned CCD sensor and so makes instantaneous measurements with high sensitivity.

Quantaurs-QY handles solution, thin-film and powder samples, and it can cool solution samples down to liquid nitrogen temperature.

Features

- Measures absolute photoluminescence quantum yield of light-emitting materials (PL measurement)
- Utilizes an integrating sphere to measure all luminous flux
- Cooled, back-thinned CCD sensor allows measurements with ultra-high sensitivity and high S/N ratio
- Automatically controls the excitation wavelengths
- Space-saving, compact design
- Wide selection of analysis functions
 - Photoluminescence quantum yield
 - Excitation wavelength dependence
 - Photoluminescence spectrum
 - PL excitation spectrum

Instantaneous measurement

The multichannel detector captures the sensitivity-compensated spectrum, and calculates the quantum yield in a process that instantaneously finds the absolute value of the quantum yield. Dialog-style dedicated software keeps the measurement process simple.

Fully automated hardware

The software-controlled monochromator allows selecting excitation wavelengths so that the sample can be excited by various excitation wavelengths. Wavelength dependence of quantum yields and excitation spectrum can then be automatically measured.


Analyzing different sample forms

Quantaaurus-QY handles solution, thin-film, and powder samples. With a Dewar flask holder, solution samples can be cooled by liquid nitrogen to -196 °C (77K).

2 models available

Two product types are provided according to the wavelength range for sample excitation and photoluminescence: one covers a spectral range from 300 nm to 950 nm and the other from 400 nm to 1100 nm.

Standard	NIR
C11347-11	C11347-12
wavelength 300 nm to 950 nm	wavelength 400 nm to 1100 nm

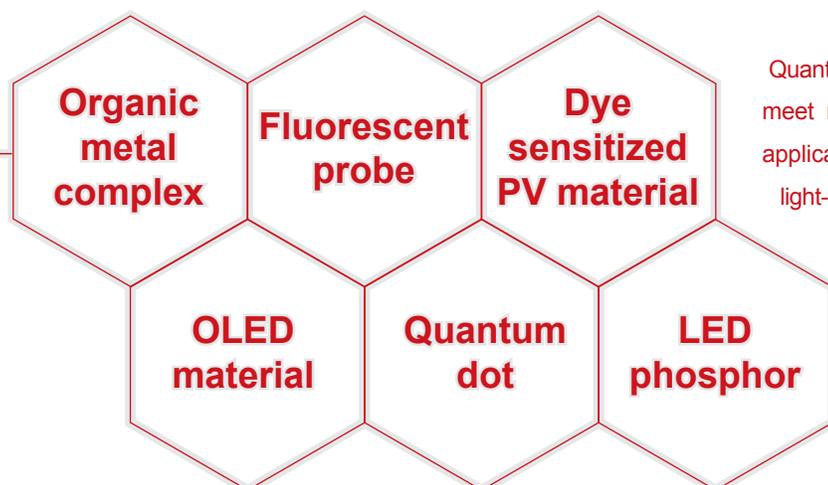

Quantum yield measurements are made in a wide range of fields to meet needs in development and research applications. Typical applications include improving quality in various types of light-emitting materials such as organic EL materials, white LED, and phosphors for FPD; researching organic metal complexes; evaluating fundamental characteristics of dye-sensitized solar cells; and measuring fluorescent probe efficiency in biological fields.

Principle of quantum yield measurement


Measurement of reference
(only for quartz cells)

Photoluminescence quantum yield

$$= \frac{\text{Number of photons emitted as photoluminescence from sample}}{\text{Number of photons absorbed by sample}}$$


Measurement of sample
(quartz cells containing sample solution)

Calculation of photoluminescence quantum yield

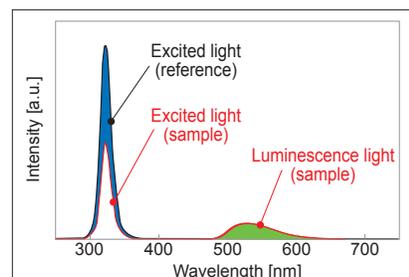


▲ Excitation light on reference and sample and photoluminescence spectrum measurement example

The dedicated software ensures simple and rapid measurements.

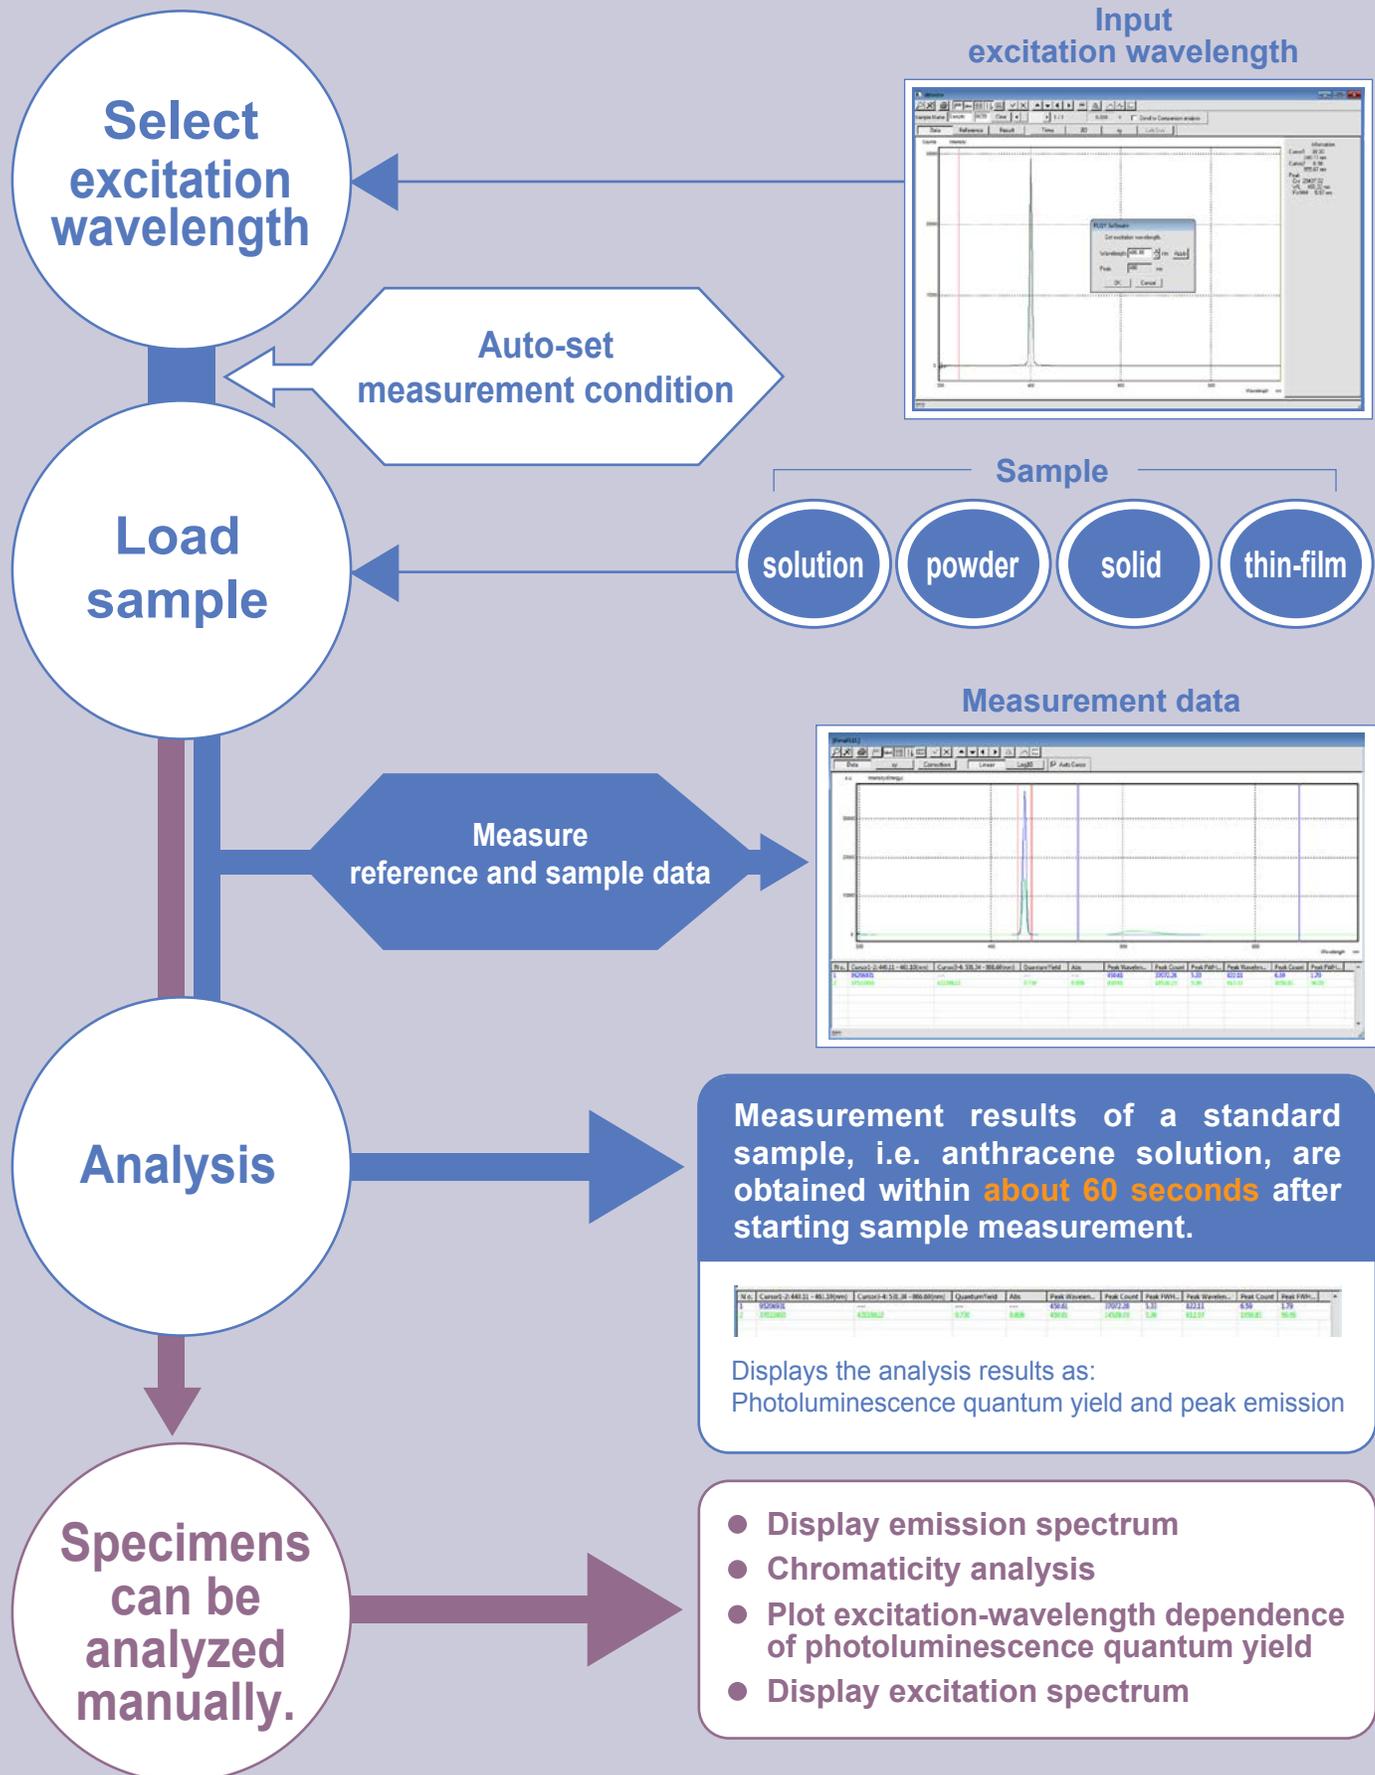


Dependence on the excitation wavelength

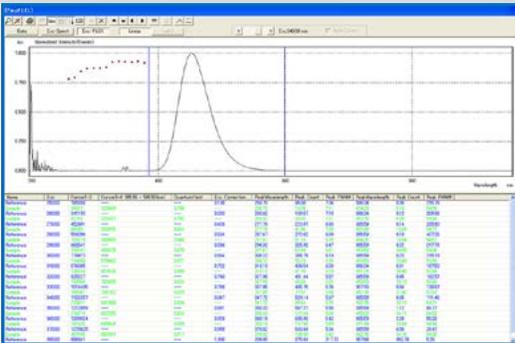


This screen shows the dependence of PL quantum yield on excitation wavelength.

PL quantum yield measurement

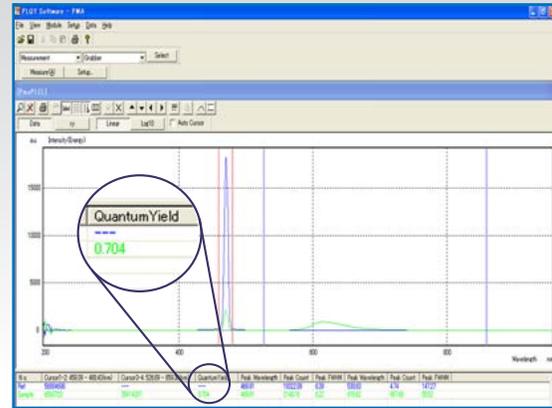


This is a basic screen for quantum yield measurements. The luminescence quantum yield is automatically calculated after measurement. Excitation and emission bands are defined by adjusting the cursors. The value of the quantum yield is displayed in the table below the spectrum next to emission intensities, peak wavelength, peak counts, and peak band (FWHM).

PL excitation spectrum

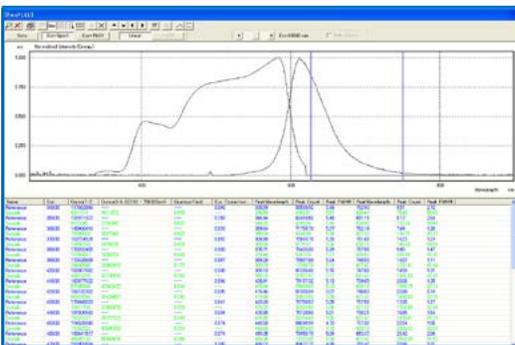


Excitation spectra can be measured by using a motorized excitation monochromator.

x-y coordinates

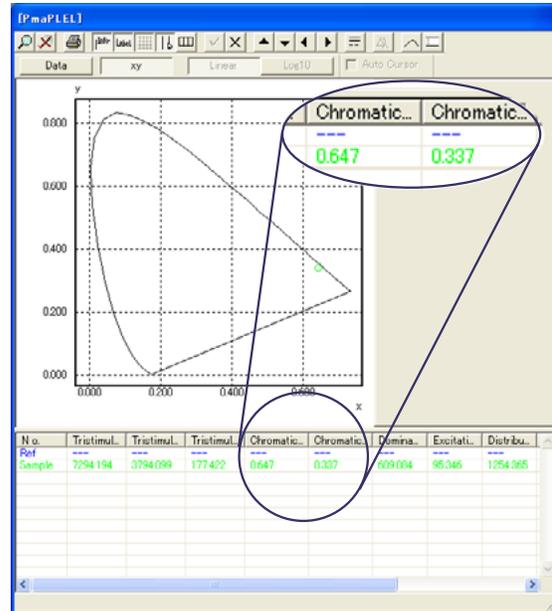


Besides displaying PL spectra and calculating quantum yields, the software also includes a function for color coordinates. Besides the chromaticity coordinates (x, y) of the measured sample, the three stimulus values (X, Y, Z) are displayed.

PL spectrum


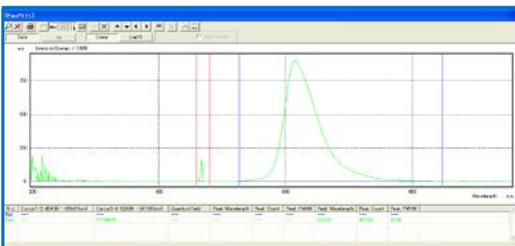


A PL spectrum is displayed after subtraction of residual excitation light components. A spectrum measured by Quantaurus-QY always contains excitation light which was not absorbed by the sample. The software offers a function for removing these remaining excitation light components and enables the user to show a purified emission spectrum.

PL quantum yield measurement of highly-fluorescent TADF materials

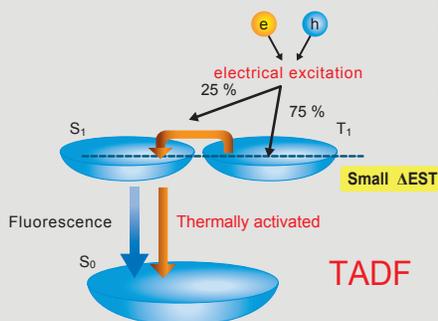


Thermally activated delayed fluorescence (TADF) materials are well known as the third generation OLED materials. TADF is the fluorescence generated by reversed intersystem crossing process (RISC) from the lowest triplet to the singlet states and the RISC is promoted by the small energy gap between the lowest excited states (Δ_{EST}). A novel TADF material (4CzIPN) was successfully developed by precise molecule design. The material has small Δ_{EST} and it shows high PL quantum yield as 0.94 +/- 0.02.

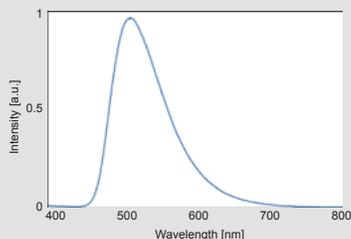

Data courtesy of Prof. Chihaya Adachi, Hajime Nakanotani, Center for Organic Photonics and Electronics Research, Kyushu Univ. Q. Zhang, B. Li, S. Huang, H. Nomura, H. Tanaka and C. Adachi, *nature photonics*, **8**, 326 (2014)

Re-evaluation of photoluminescence quantum yield of representative standard solutions

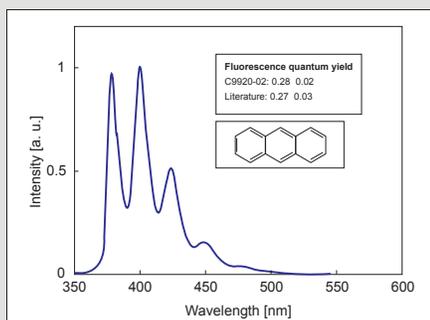


The quantum yields of fluorescence standard solutions were measured with our Absolute PL quantum yield measurement system. The fluorescence standard solutions have been used for determining PL quantum yield based on a relative method. For the most compounds, the quantum yield measured by our system shows excellent agreement with the values given in the literature, proving the high reliability of our system.

Figure: Fluorescence spectrum and quantum yield of anthracene solution


Collaborative research of Hamamatsu Photonics K.K.; A. Kobayashi, S. Kaneko, K. Takehira, T. Yoshihara, and S. Tobita, Faculty of Engineering, Gunma University; H. Ishida, Y. Shiina, and S. Oishi, School of Science, Kitasato University K. Suzuki, A. Kobayashi, S. Kaneko, K. Takehira, T. Yoshihara, H. Ishida, Y. Shiina, S. Oishi, and S. Tobita, *Phys. Chem. Chem. Phys.*, **11**, 9850 (2009).

Quantum yield measurement of fluorescent bioprobe

Fluorescent probe for enzyme reaction detection: Quantum yield provides a comparative measurement.

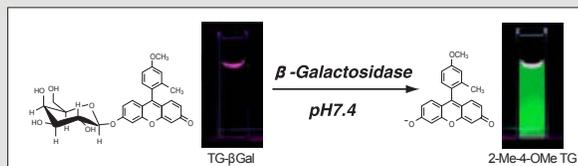

Compounds	Fluorescence quantum yield
TG-βGal	0.01
2-Me-4-OMe TG	0.72

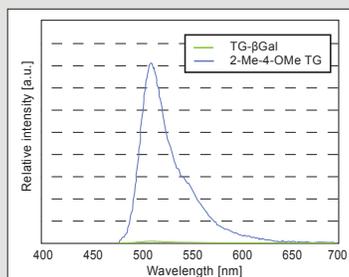

Fluorescent probe TG (Tokyo Green) -βGal for β-galactosidase activity detection is nonluminescent ($\Phi_f = 0.01$) but exhibits strong fluorescence after reacting with β-galactosidase. The quantitative difference in amounts of light emitted before and after the enzyme reaction can be found by comparing their quantum yields Φ_f .

Data courtesy of Yasuteru Urano, Ph.D., Graduate School of Medicine, the University of Tokyo.

Fluorescence Lifetime and Absolute PL Quantum Yield

There are two processes when substances are excited by light irradiation from the ground state to excited singlet state (S1), then deactivated to the ground state again. One is radiative process such as fluorescence or phosphorescence, and the other one is a non-radiative process released as heat.

The fluorescence lifetime τ (tau) is defined as

$$k_f + k_{nr} = 1/\tau$$

where k_f is the radiative rate constant and k_{nr} is the non-radiative constant.

On the other hand, the PL Quantum Yield (Φ) is expressed as the ratio of the number of photons emitted from molecules (PN_{em}) to that absorbed by molecules (PN_{abs}).

$$\Phi = PN_{em} / PN_{abs}$$

However the PL Quantum Yield Φ is also written as

$$\Phi = k_f / (k_f + k_{nr})$$

Thus, there is a close relationship between $\Phi(\tau)$ and Φ as shown in the following equation, and they are very important parameters for controlling the emission mechanisms of the materials.

$$k_f = \Phi / \tau$$



A diversified evaluation of the luminescence materials is now available!

Newly developed Quantaurs-Tau for measuring fluorescence lifetime and Quantaurs-QY for absolute PL quantum yield with simplified and minimized operating procedure are now available for everybody. Combination of Quantaurs-Tau and Quantaurs-QY allow users to obtain complementary analysis results.



Fluorescence lifetime spectrometer C11367 series



Absolute PL quantum yield spectrometer C11347 series



Specifications

Type number	C11347-11 (Standard type)	C11347-12 (NIR type)
PL measurement wavelength range	300 nm to 950 nm	400 nm to 1100 nm
Monochromatic light source		
Light source	150 W xenon light source	
Excitation wavelength	250 nm to 850 nm	375 nm to 850 nm
Bandwidth	10 nm or less (FWHM)	
Excitation wavelength control	Automatic control	
Multichannel spectroscopy		
Measurement wavelength range	200 nm to 950 nm	350 nm to 1100 nm
Wavelength resolution	<2 nm	<2.5 nm
Number of photosensitive device channels	1024 ch	
Device cooling temperature	-15 °C	
AD resolution	16 bit	
Spectroscopy optical arrangement	Czerny-Turner type	
Integrating sphere		
Material	Spectralon	
Size	3.3 inch	
Software		
Measurement items	PL quantum yield	
	Excitation wavelength dependence of quantum yield	
	PL spectrum (peak wavelength, FWHM)	
	PL excitation spectrum	
	Color measurement (chromaticity, color temperature, color rendering index, etc.)	

Options

Sample holder

For solution

- Sample holder for low temperature A11238-04

For powder

- Sample holder for temperature control A9924-17

This option allows setting the maximum temperature of powder samples up to 180 °C. Measurements can now be made in environments where phosphors for white LED are actually used. Temperature control range: RT to +180 °C.

Sample case

For solution

- Side-arm cell (3 sets) A10095-02
 - Sample tube for low temperature measurement (5 pcs) A10095-04
- This is used to measure a sample solution at liquid nitrogen temperature.

For powder

- Laboratory dish without caps (5 sets) A10095-01
- Laboratory dish with caps (5 sets) A10095-03


This is used for making measurements on powder samples. This is a five-piece set made of synthetic quartz, which suppresses fluorescence and luminescence.



Others

- Precision temperature controller C13453
- The unit controls temperature of sample holder A9924-17.

Dimensional outlines (Unit: mm) Weight: Approx. 26.5 kg

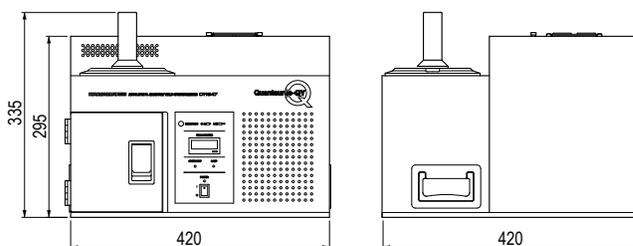

Quantaurs-QY is registered trademark of Hamamatsu Photonics K.K. (EU, Korea, Japan, U.S.A.)

Quantaurs-Tau is registered trademark of Hamamatsu Photonics K.K. (EU, Korea, Japan, U.S.A.)

Product and software package names noted in this documentation are trademarks or registered trademarks of their respective manufacturers.

- Subject to local technical requirements and regulations, availability of products included in this promotional material may vary. Please consult your local sales representative.
- Information furnished by HAMAMATSU is believed to be reliable. However, no responsibility is assumed for possible inaccuracies or omissions. Specifications and external appearance are subject to change without notice.

© 2016 Hamamatsu Photonics K.K.

HAMAMATSU PHOTONICS K.K. www.hamamatsu.com

HAMAMATSU PHOTONICS K.K., Systems Division

812 Joko-cho, Higashi-ku, Hamamatsu City, 431-3196, Japan, Telephone: (81)53-431-0124, Fax: (81)53-435-1574, E-mail: export@sys.hpk.co.jp

U.S.A.: Hamamatsu Corporation: 360 Foothill Road, Bridgewater, NJ 08807, U.S.A., Telephone: (1)908-231-0960, Fax: (1)908-231-1218 E-mail: usa@hamamatsu.com

Germany: Hamamatsu Photonics Deutschland GmbH: Arzbergerstr. 10, D-82211 Herrsching am Ammersee, Germany, Telephone: (49)8152-375-0, Fax: (49)8152-265-8 E-mail: info@hamamatsu.de

France: Hamamatsu Photonics France S.A.R.L.: 19, Rue du Saule Trapu, Parc du Moulin de Massy, 91882 Massy Cedex, France, Telephone: (33)1 69 53 71 00, Fax: (33)1 69 53 71 10 E-mail: infos@hamamatsu.fr

United Kingdom: Hamamatsu Photonics UK Limited: 2 Howard Court, 10 Tewin Road, Welwyn Garden City, Hertfordshire AL7 1BW, UK, Telephone: (44)1707-294888, Fax: (44)1707-325777 E-mail: info@hamamatsu.co.uk

North Europe: Hamamatsu Photonics Norden AB: Torshamnsgatan 35 16440 Kista, Sweden, Telephone: (46)8-509-031-00, Fax: (46)8-509-031-01 E-mail: info@hamamatsu.se

Italy: Hamamatsu Photonics Italia S.r.l.: Strada della Moia, 1 int. 6, 20020 Arese (Milano), Italy, Telephone: (39)02-935-81-733, Fax: (39)02-935-81-741 E-mail: info@hamamatsu.it

China: Hamamatsu Photonics (China) Co., Ltd.: 1201 Tower B, Jianning Center, 27 Dongshanhuan Beilu, Chaoyang District, 100020 Beijing, China, Telephone: (86)10-6586-6006, Fax: (86)10-6586-2866 E-mail: hpc@hamamatsu.com.cn

Taiwan: Hamamatsu Photonics Taiwan Co., Ltd.: 8F-3, No. 158, Section2, Gongdao 5th Road, East District, Hsinchu, 300, Taiwan R.O.C. Telephone: (886)03-659-0080, Fax: (886)07-811-7238 E-mail: info@tw.hpk.co.jp